

Ordering the Slide

Two Versions. Same Comfort Design.

The Slide’s unique product line of *soft-tissue friendly* devices for sleep apnea and snoring is available in two versions, made from different materials.

The Slide® Nylon: Made with type 12 nylon and 3D printed for super strength

The Slide® Acrylic: Made with KeySplint Soft 3D printed resin for flexibility

Both are ideal for treating the majority of sleep apnea and snoring conditions.

the Slide® Nylon



Super Strong

the Slide® Acrylic



Flexibility


TO UPLOAD A NEW PATIENT CASE

1. Create your account in the Slide [Customer Portal](#)
2. Add Slide Sleep Technologies to your scanner.

Note: We currently partner with Itero Lab ID #23008, Medit, Trios (3 Shape Communicate) and Carestream/Dexis.

If using a Sirona (Cerec) scanner please convert scans to STL files and upload them on the customer portal.

3. Scan your patient's upper and lower arches, being sure to include the distal wrap of the last molars.
 - Check your patient's midline to insure they line up and please note if there is a discrepancy for any midline shift.
 - ONLY the protrusive bite is required. A minimum clearance of 5mm over the posterior teeth is required for connector placement. We have the ability to open the bite minimally to accommodate any lack in vertical clearance.
 - Do not send a C.O. bite.

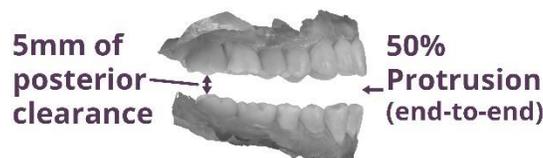

theSlide_OG_23321

4. Upload your scans

- If your scanner is not listed, you can log into your account on the Slide Customer Portal and click on the "Cases" button, next to the "Submit a Case" button.
- Under **Products**, select which Slide device you would prefer, and Upper and Lower Arches if original submission. If replacing one arch, select which arch.
- Under **Attachments**, select "Digital Impressions" button, export your STL file, and Drop and Drag it into the field.


5. If you are not using Digital Scans, we can accept PVS impressions. They must include the distal wrap of the last molars. Follow the steps on the bite above using bite registration material. No wax bites please.

- Click here for [the Slide RX Form](#)
- Sign-into the Slide [Customer Portal](#) to generate a mailing label
- Send off your impressions using the mailing label

FOR TRADITIONAL PVS IMPRESSIONS

1. Download the Prescription: [the Slide RX Form](#)
2. Indicate the version of the Slide you are ordering by checking one of the following boxes on the Prescription Form:
3. Make sure the distal of all most posterior teeth are captured.
4. Please note the bite clearance. A minimum clearance of 5mm over the posterior teeth is required for connector placement.

- theSlide^z
- The Slide Nylon**
(Made with Type 12 Nylon, SLS, 3D printed)
 - The Slide Acrylic**
(Made with KeySplint Soft 3D printed resin)

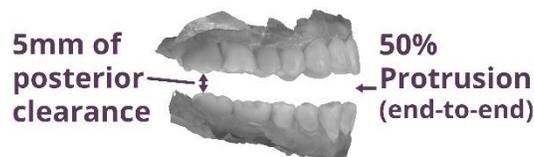

5. Send impressions, bite, and prescription to:

Slide Sleep Technologies
114 Holmes Road, Suite 146
Houston, TX 77045

6. Sign-into the Slide [Customer Portal](#) to generate a mailing label

FOR ASSISTANCE

Call Toll Free: 1-855-754-3311
Email: info@slide2sleep.com